

# REVISTA CIENTIFICA

## Volumen 01-07

### COLEGIO DE QUIMICOS DE PUERTO RICO

# EL CRISOL

#### Junta de Gobierno 2006-2007

Presidenta

Lcda. Rebecca Soler

Presidenta Electa

Lcda. Monserrate Santiago

Secretario

Lcdo. Héctor J. Acosta

Tesorero

Lcdo. Ángel Marrero

Pasada Presidenta Inmediata

Lcda. María E. Ramírez

Delegados:

Academia

Dra. Agnes Costa

Dra. Ethel Ríos

Gobierno

Lcda. Ivette Irizarry

Lcdo. Raymond Frye

Privado

Lcdo. Edwin Medina

Industrial

Lcdo. Luis Rivera

Lcdo. Harry Acosta

Lcda. Sonia Pichardo

Lcda. Flor V. Chinae



Teléfonos: 787-763-6070 / 763-6076

Fax: 787-758-2615

Webpage: [www.cqpr1941.org](http://www.cqpr1941.org)

E-mail: [cqpr@cqpr1941.org](mailto:cqpr@cqpr1941.org)

## **Microfluidic bioreactors as tools for monitoring cell microenvironment**

**Miguel A. Acosta, Yordan Kostov, and Jennie B. Leach** *Department of Chemical & Biochemical Engineering, University of Maryland-Baltimore County*

**Statement of purpose:** Understanding the mechanisms underlying cell response to cues from their biomaterial microenvironment will ultimately lead to improved methods to control cell behavior in tissue replacement therapies. Whereas many methods have been established for characterizing cellular behavior and physical properties of biomaterial scaffolds, few methods exist for quantitatively mapping the fluctuations of soluble cues that impact cellular function. *Our overall goal* is to develop an integrated microfluidic bioreactor/sensor system to investigate cell response to changes in the chemical microenvironment found within 3D biomaterial scaffolds. *Our current work* focuses on developing novel technologies for sensing spatial and temporal changes in oxygen content during 3D culture. Oxygen is required for the aerobic metabolism of carbon compounds in cells and as such is a critical parameter (along with pH, temperature, and nutrient supply) that impacts cell viability. Furthermore, oxygen tension itself is a cue that directly impacts cell response (e.g., migration). Measurements of oxygen concentration in microfluidics systems are difficult because traditional oxygen-sensing approaches are not amenable to miniaturization. Moreover, oxygen-sensing electrodes also consume oxygen during operation. We present the development of an oxygen sensor based on fluorescence quenching of PDMS-embedded tris (4,7-diphenyl-1,10-phenanthroline) ruthenium (II) dichloride. By monitoring the quenching of this oxygen sensitive fluorescent dye, measurements of oxygen concentration can be carried out in a non-invasive manner without consuming the oxygen available to the cells during culture. Results from microfluidic bioreactor fabrication and oxygen sensor calibration are presented.

**Methods:** *Fabrication of microfluidic bioreactor.* Soft lithography was used to fabricate the bioreactor as previously described by Whitesides and coworkers [1]. To fabricate the master, photoresist was patterned on 2.54 cm x 2.54 cm microscope slides. PDMS (20:1 elastomer:curing agent) was poured over the master and cured overnight. The PDMS replica was oxidized and sealed to a clean glass slide, also 2.54 cm x 2.54 cm. 0.58 mm-ID polyethylene tubing was connected via incisions made with a 1 mm blunt syringe (Fig. 1). *Oxygen sensor sample preparation.* PDMS was similarly prepared and cut into 3 cm x 1 cm x 0.2 cm pieces. The PDMS pieces were pre-swelled by submerging in dichloromethane for 10 min. Afterwards, the PDMS samples were submerged in a solution of 0.5 mm fluorescent ruthenium dye in dichloromethane for 3 or 9 min ( $n = 3$  each).



**Figures:** (1) Photograph of microfluidic bioreactor. Microchannel dimensions are 200  $\mu$ m x 200  $\mu$ m x 1 cm (width, depth, and length).

Teléfonos: 787-763-6070 / 763-6076


Fax: 787-758-2615

Webpage: [www.cqpr1941.org](http://www.cqpr1941.org)

E-mail: [cqpr@cqpr1941.org](mailto:cqpr@cqpr1941.org)

### Fluorescence measurements.

Fluorescence kinetics measurements were carried out in a Varian Cary Eclipse fluorescence spectrophotometer (470 nm excitation and 610 nm emission). Kinetics measurements were taken every 0.6 s for 1 h while the oxygen content of the atmosphere surrounding the samples was varied using mixtures of air and nitrogen gas (Fig. 2). Schematic of kinetics experiment.

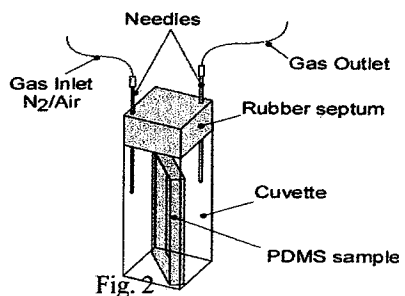

### Results/Discussion:

**Characterization of bioreactor.** A wide range of flow rates (from 0.001 to 5 mL/min) was achieved in the bioreactor using water. For flow rates up to 1 mL/min, Reynolds numbers ranged from 4.2 to 83.2, indicating laminar flow. Shear stresses at the walls of the microchannel ranged from 9.4 to 187.5 dyn/cm<sup>2</sup>. **Sensor calibration.** The decrease in intensity of the fluorescent dye can be related to the concentration of the quencher by using the Stern-Volmer equation [2, 3]. The sensitivity [1.10 S<sub>0</sub>/I<sub>0</sub>] was plotted with respect to oxygen content (assumed to be 21% in air) (Fig 3).

Results shown in Fig. 3 are means +/- standard deviation. Data were compared using a Student's t-test. The values of sensitivity were considered significantly different if  $p < 0.05$ . The mean values of sensitivity with varying oxygen content for the 3-min and the 9-min samples were found to be not significantly different ( $p > 0.05$ ).

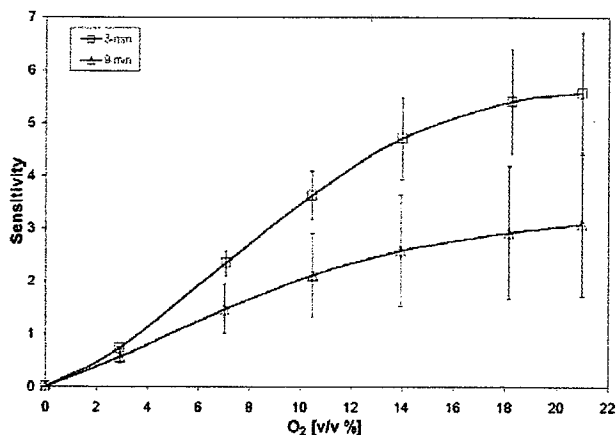


Fig 3

**Conclusions:** A microfluidic bioreactor was fabricated using PDMS and glass slides. A wide range of volumetric flow rates was achieved under laminar conditions. We have also demonstrated the oxygen sensor system based on fluorescent ruthenium dye embedded in PDMS is able to detect changes in oxygen content of 0 to 21% in air. Current work focuses on monitoring oxygen content in liquid solutions and fabricating the microfluidic bioreactor with the oxygen-sensing ruthenium dye embedded in the channel walls. Future work focuses on determining cellular viability under normoxic and hypoxic conditions within the microfluidic bioreactor as well as 3D scaffolding biomaterials.

**References:** [1] Whitesides G.M., et al., *Electrophoresis*, 2000. 21(1): p 27-40. [2] Bacon, J.R and Demas, J.N., *Anal Chem*, 1987. 59: p. 2780- 2785. [3] Kneas K.A., et al., *Applied Spectroscopy*, 1997. 51(9): p. 1346- 1351.

**Acknowledgments:** People: The UMBC Chemical and Biochemical Engineering Department and Maryland's PROMISE Director, Dr. Renetta Tull. Financial support: NSF LSAMP Bridge to the Doctorate Fellowship (to MAA) and the Clare Boothe Luce Professorship (to JBL).

Teléfonos: 787-763-6070 / 763-6076

Fax: 787-758-2615

Webpage: [www.cqpr1941.org](http://www.cqpr1941.org)

E-mail: [cqpr@cqpr1941.org](mailto:cqpr@cqpr1941.org)